

### **Learner Outcomes**



 After this session, participants will be able to do the following things

- Program Sonic hearing aids on the EXPRESSfit® Pro 2019.2 software platform
- Transfer hearing instrument settings from one style of hearing aid to a different style hearing aid using the Transfer Settings tool in the EXPRESSfit® Pro fitting software
- Update firmware on Sonic hearing aids, using the Firmware Updater tool.

www.sonici.com

SONIC Everyday Sounds Better


## New! in EXPRESSfit® Pro 2019.2



- Support for new Trek products:
  - 2 Technology levels
    - Trek 80 | 40
  - 2 form factors
    - Super Power and Ultra Power BTEs
- Updated Transfer Fitting feature
- Bimodal fitting support
- Firmware update

www.sonici.com

((C SONIC ))) Everyday Sounds Better

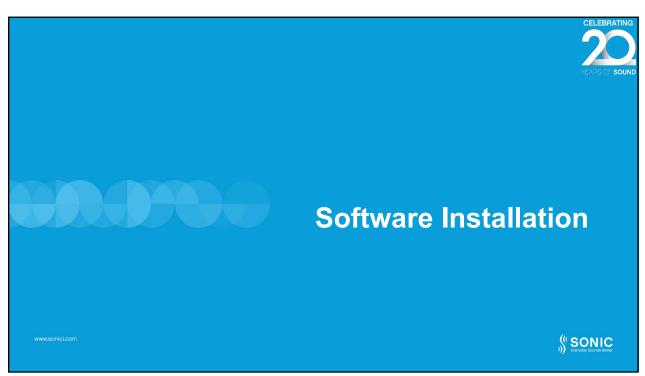

# Website Download • Download and install from the website: • www.sonici.com • Go to Professional Center Find what you need for fitting You're about to experience how easy fitting a Sonic device can be.



## **Sonic Software Updater**



- Open in task bar or All Programs
  - Cannot be opened from EXPRESSfit® Pro
- Downloads in the background
- OK to turn off PC, download will resume when powered up again
- Install prompt will appear when download completes
- Download is deleted after install

www.sonici.com

SONIC Everyday Sounds Better


7


### CELEBRATING **Sonic Software Updater** Changing the settings of the updater Automatically download updates Automatically install updates Automatically download Update check interval updates Start EXPRESSfit Updater with Windows Automatically install Preferences updates Check for update Check for interval Cancel download updates Start installation Delete downloaded update Cancel, install and delete download from Exit this menu www.sonici.com SONIC







# Firmware Updater – What Is It? • Updates hearing instruments and accessories with • New features • Security updates • Fixes so repairs can be made in the clinic

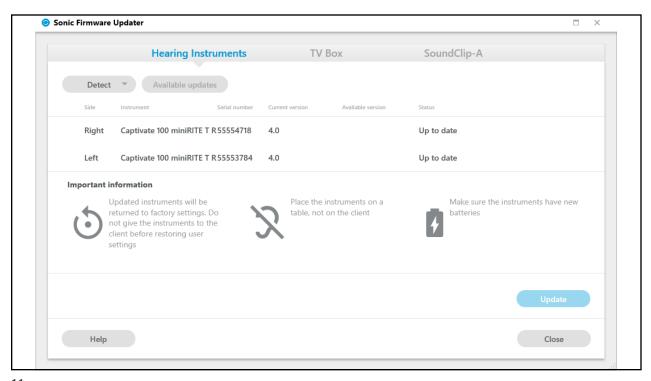

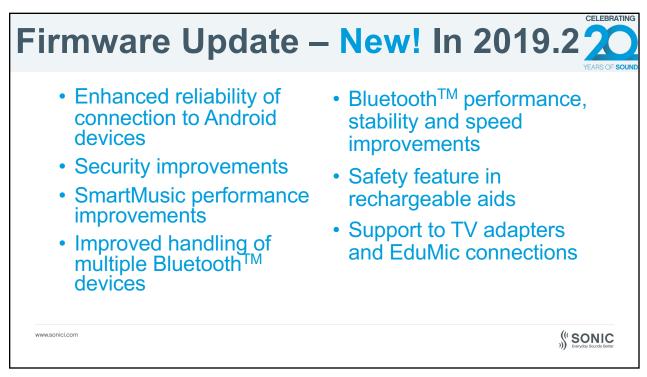

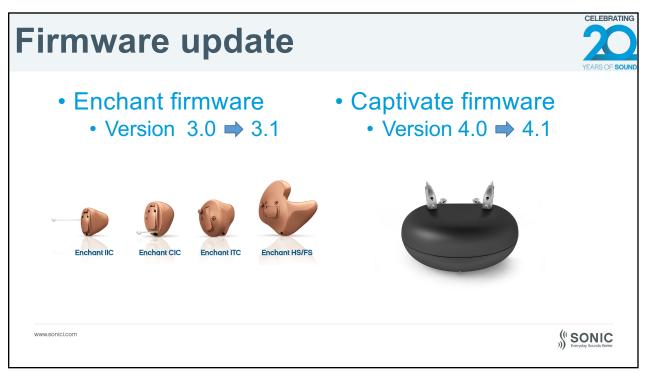

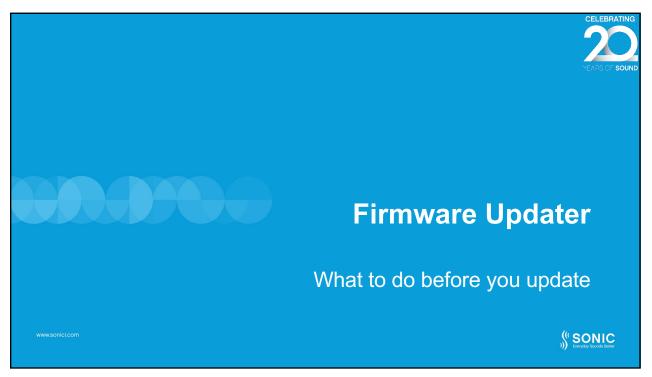


### **Before You Update**



- The following scenarios must be met
  - Computer is online
  - Use a hardwire connection
    - Captivate miniRITE T R requires red pin removal tool to open battery drawer for hardwire connection
  - Use fresh/fully charged batteries
    - Ensure > 11% charge for the Captivate miniRITE T R
  - It is recommended that programming is saved before doing a firmware update

www.sonici.com




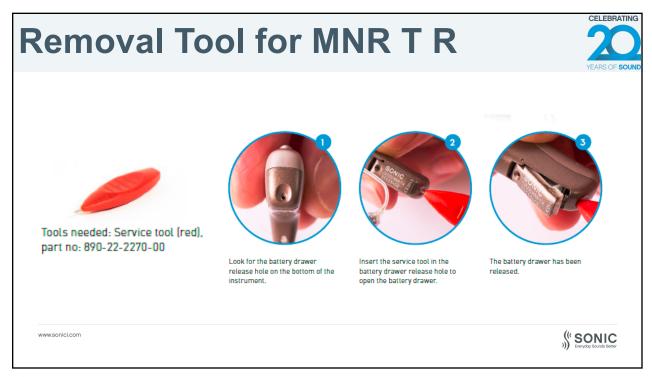





CELEBRATING **Open Firmware Updater** • EXPRESSfit® Pro Windows Start Menu Click Tools in menu bar · Scroll down to 'All Programs' Click Sonic Firmware · Click on the Sonic folder Updater • Click Sonic Firmware Updater Sonic Test box measurement EXPRESSfit Pro Launch Sonic Firmware Updater EXPRESSfit Sonic Firmware Updater Sonic Updater Preferences www.sonici.com SONIC Sounds Rether

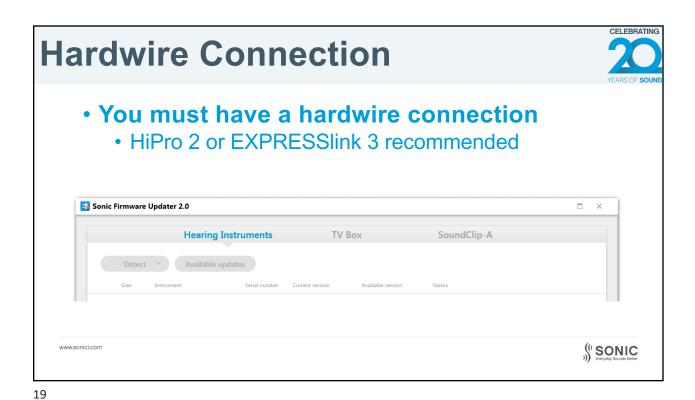

Detect in Firmware Updater

 Select a programming device

 Click Detect
 Sonic Firmware Updater 2.0

 Hearing Instruments
 TV Box SoundClip-A

 Detect Sound Struments
 No Instruments detected To detect instruments, use a cable connection

NOAHlink H-9RO Usb To detect instruments, use a cable connection


WWW.sconicl.com


\*\*CELEBRATING STRUMENTS\*\*


\*\*CARSO C SOUND

\*\*CONIC FIRMWARE Updater 2.0

\*\*CO

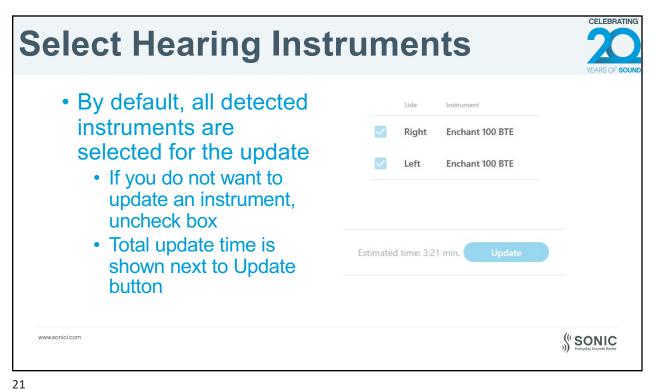

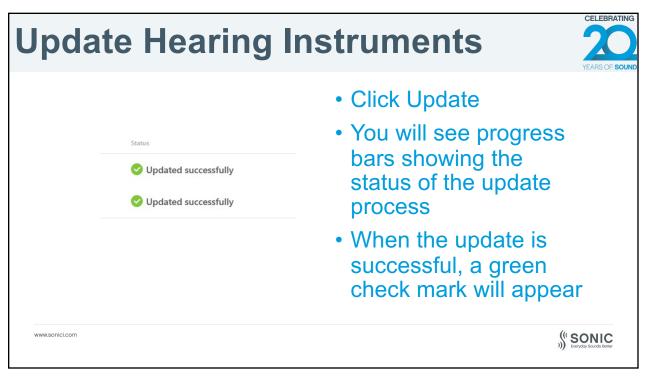

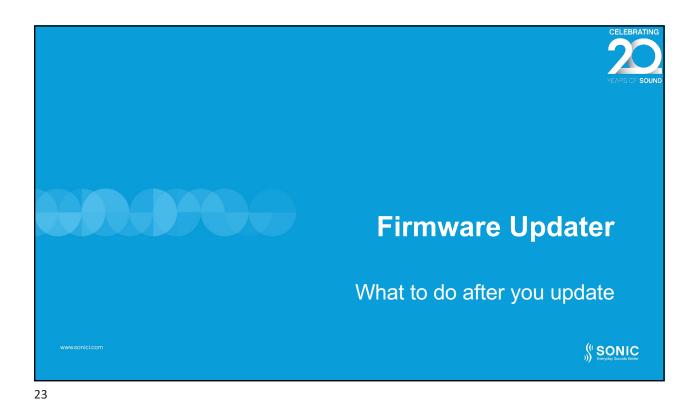

## **After You Update**




- You Must Restore Patient Settings!!!
  - Updated instruments are returned to factory settings after update
  - Read instruments in EXPRESSfit® Pro directly after update, choose 'use session data' when prompted to restore user settings
  - It is recommended that the hearing instruments are hardwired for restoring session data

www.sonici.com






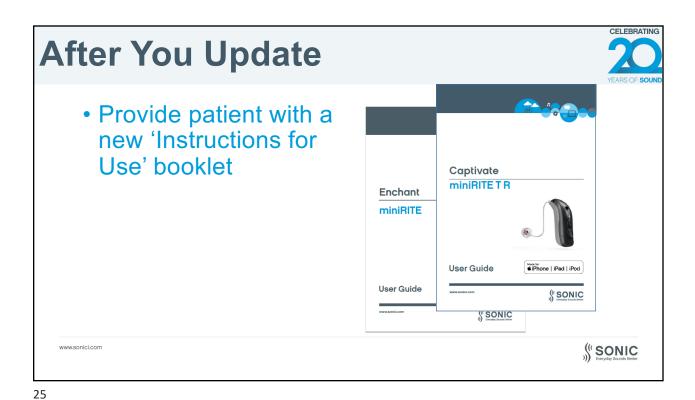

Transfer Settings

What's new in EXPRESS fit® Pro 2019.2

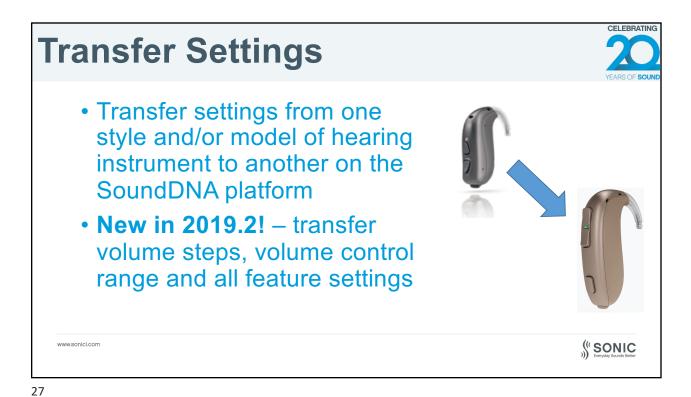

CELEBRATING **Transfer Settings**  When you connect an instrument in a patient record that has a saved session from a different style or technology level on the SoundDNA platform, there will be a prompt with an option to use the Transfer Settings tool to transfer patient settings Fitting data conflict Fitting data conflict The current fitting session data differs from the detected instrument settings. The current fitting session data differs from the detected instrument settings. Choose how to proceed: Choose how to proceed: Use hearing instrument data Use hearing instrument data O Start new fitting O Start new fitting CV100 MNR T R 85 CV100 MNR T R 85 O Use session data (Transfer Fitting) Use session data (Transfer Fitting) Continue www.sonici.com SONIC

### **Transfer Settings**



 A screen will appear next, explaining what will be transferred and what will be removed and prescribed

### Will be transferred

 All settings available with the same values on source and target instruments


### Will not be transferred


- Feedback measurements
- In-situ audiometry results
- Accessories pairing
- Settings that are not available in the target instruments
- Settings which cannot be transferred correctly.

These settings will be set to default, or they will be prescribed

www.sonici.com


SONIC Everyday Sounds Better

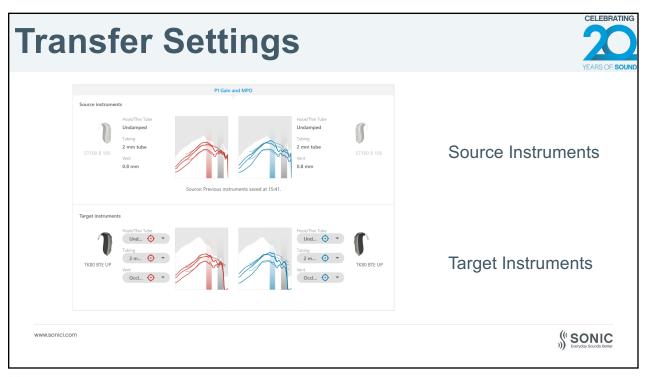


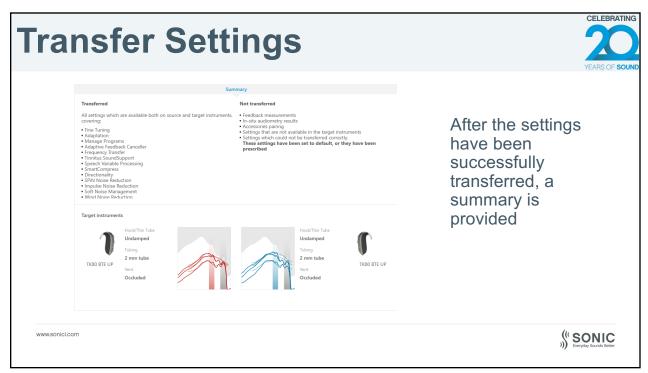






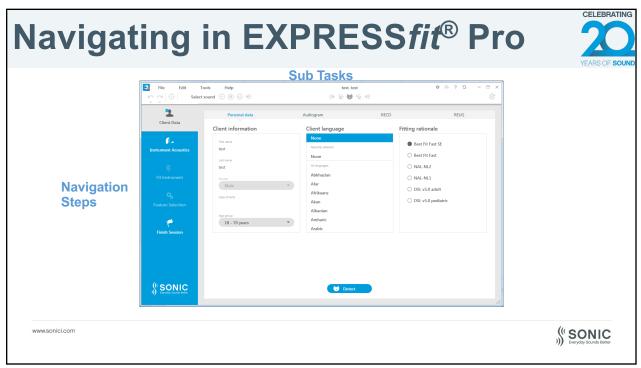

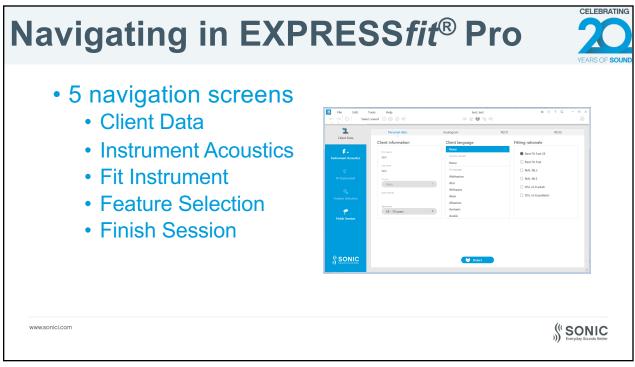

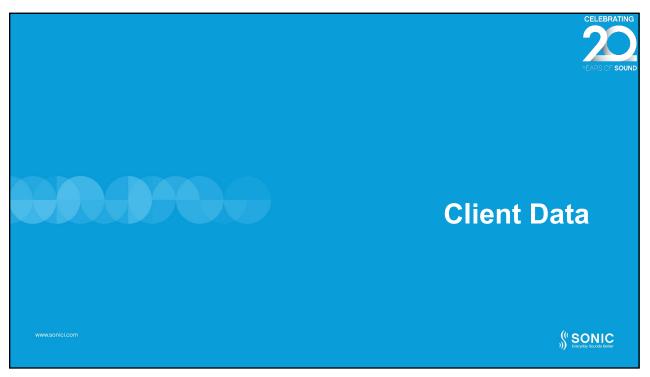

## **Client Data**




- Check demographic data
  - Add gender and age if needed
- Select appropriate language
- Tabs for Audiogram, RECD and REUG information
- In-Situ Audiometry available (Audiogram)


www.sonici.com


SONIC Everyday Sounds Better


37


### CELEBRATING **Supported Fitting Algorithms** Best Fit Fast Fitting Rationale Designed to guickly achieve a good fitting result Best Fit Fast Emphasizes speech intelligibility while still providing comfort Best Fit Fast SE NAL-NL1 Best Fit Fast SE ○ NAL-NL2 Emphasizes speech intelligibility for experienced ○ DSL [i/o] O DSL 5 Adult users **Default for Trek!** Great choice for patients who prefer fittings with O DSL 5 Child more gain SONIC www.sonici.com

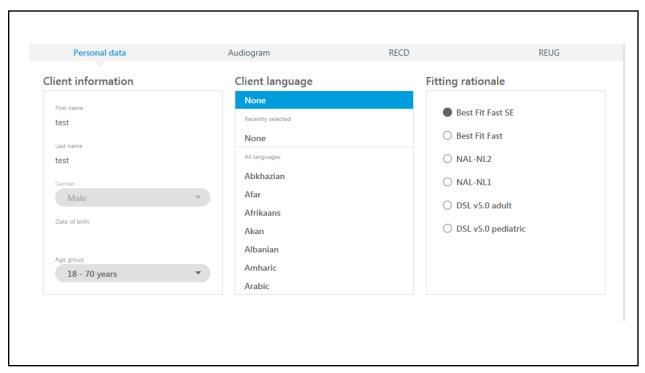


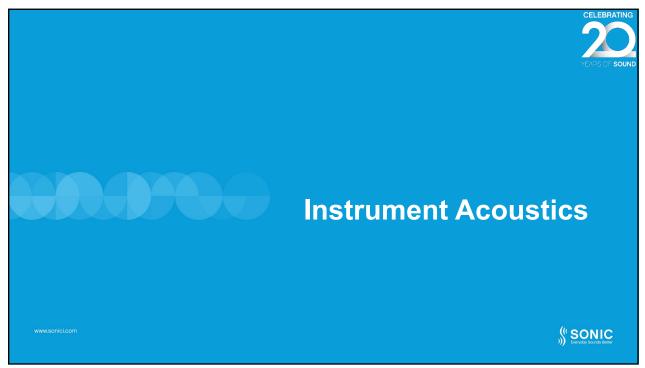

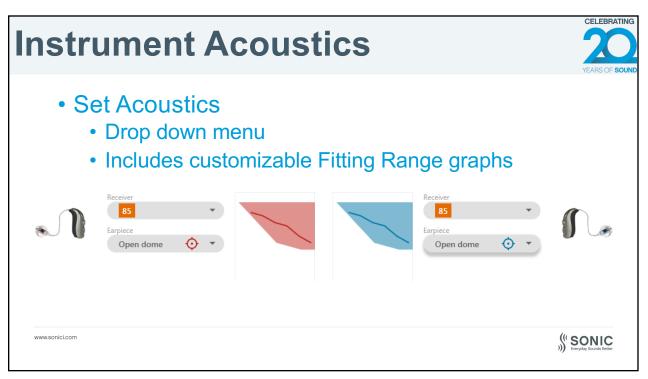


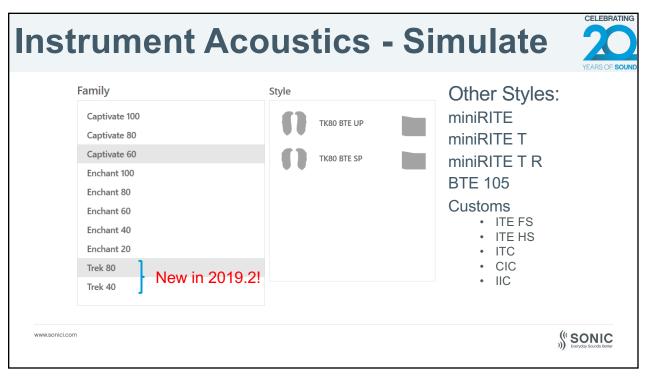


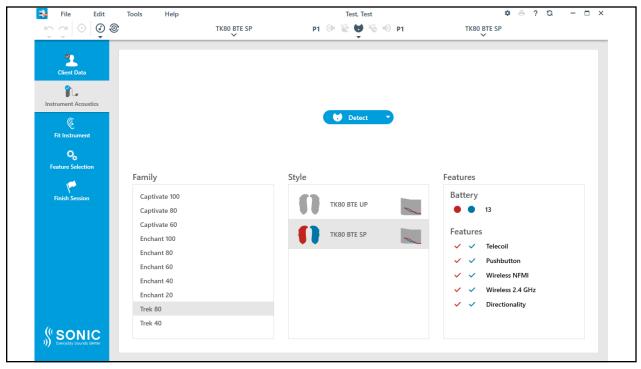


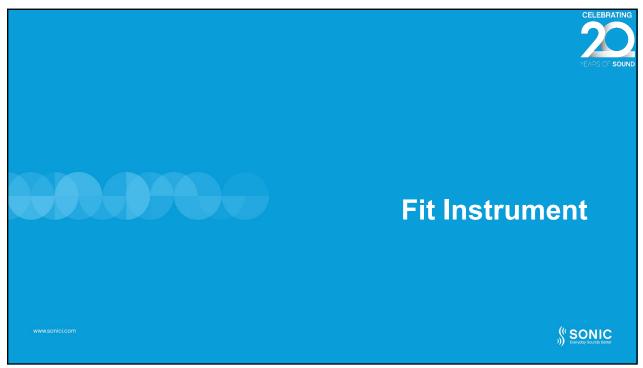





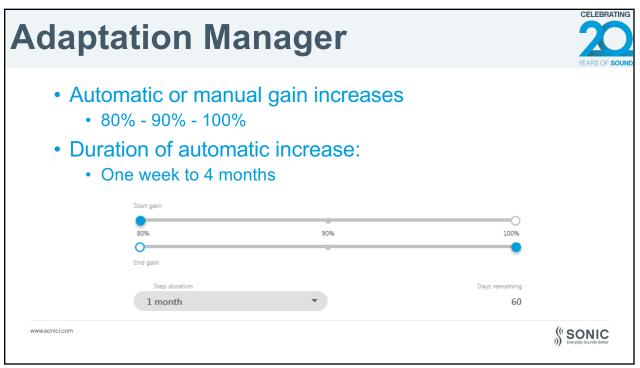

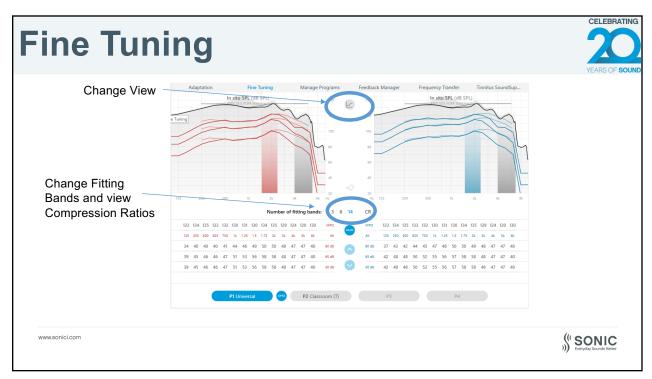

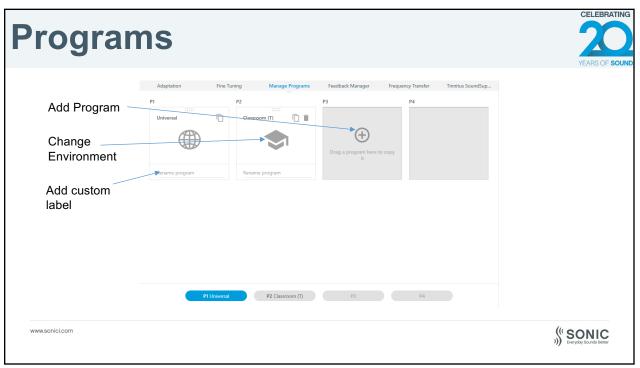

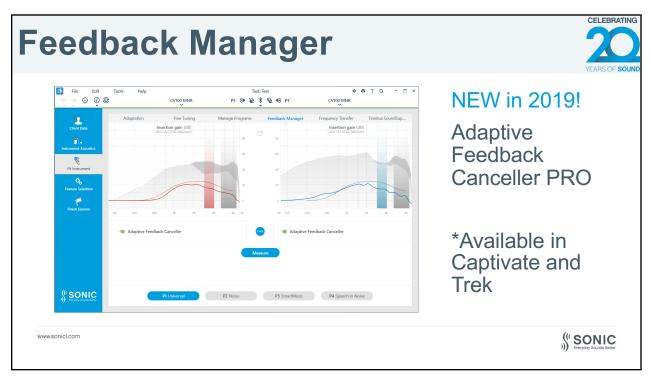

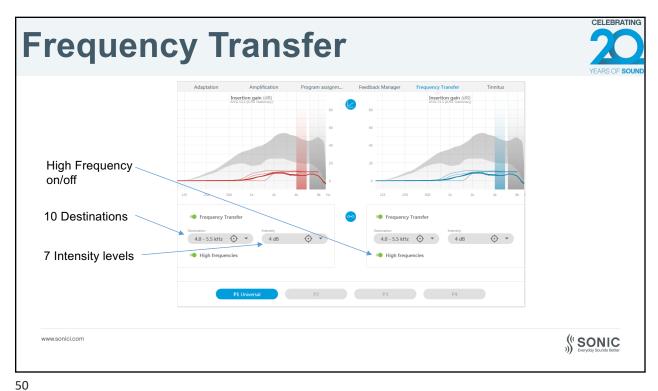


### **Tinnitus SoundSupport**





- Adjust Tinnitus signal:
  - White Noise, Pink Noise etc...
- Add modulation
- Add automatic level steering
  - Level of signal adjusts base on environment
- Turn off Hearing Aid microphone


www.sonici.com


SONIC Everyday Sounds Better

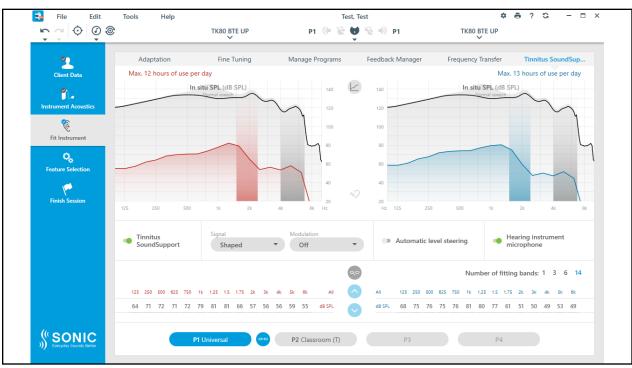


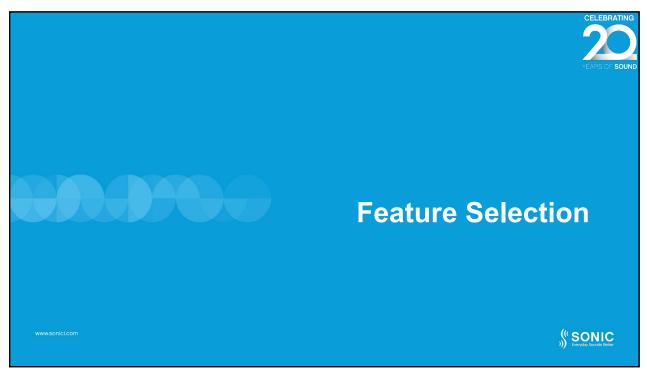


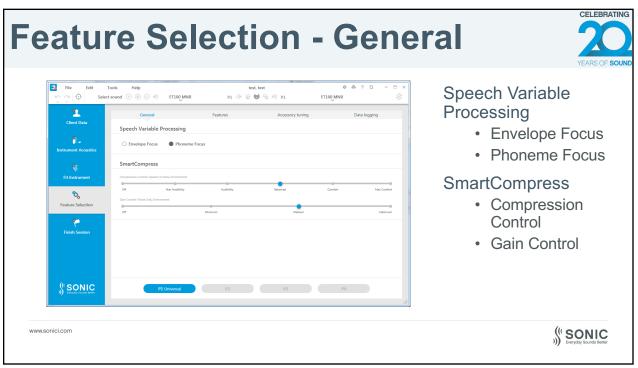


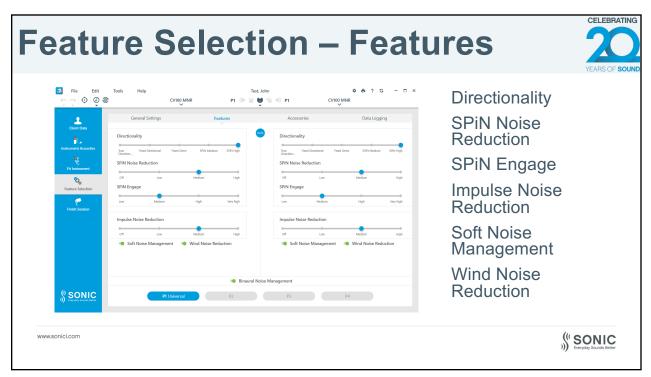


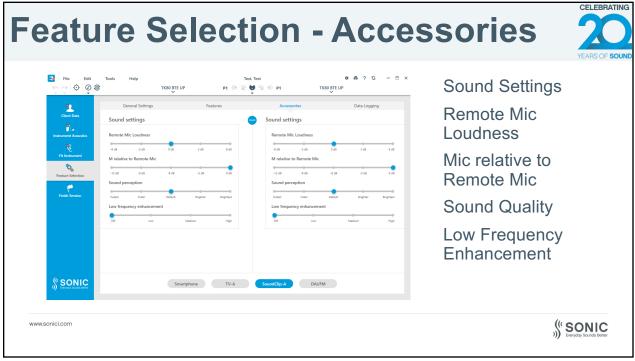


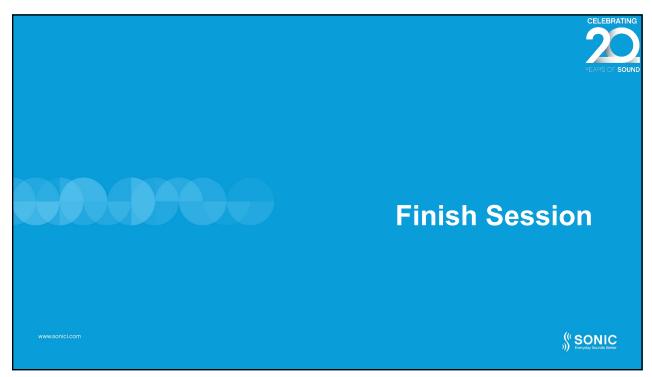


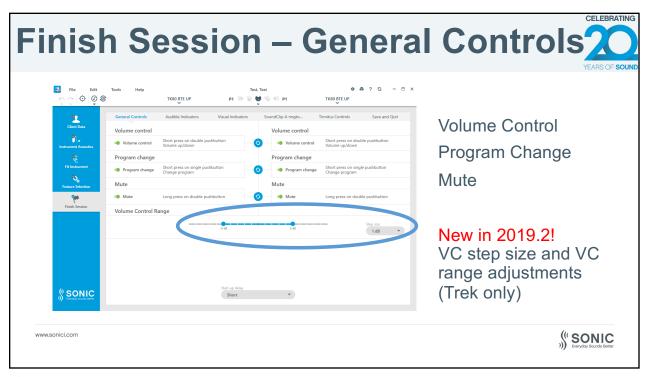


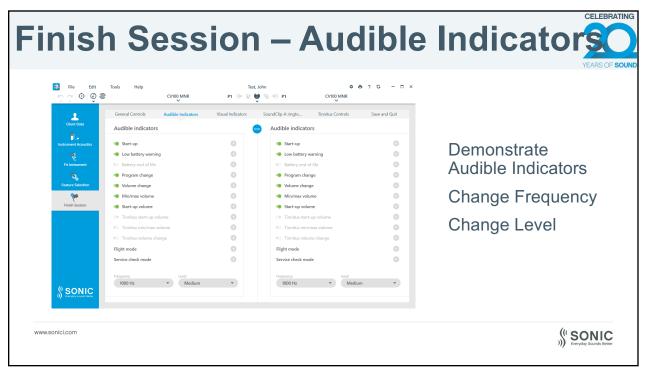


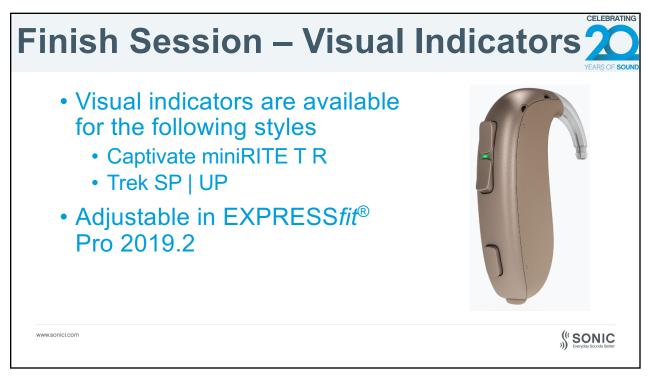


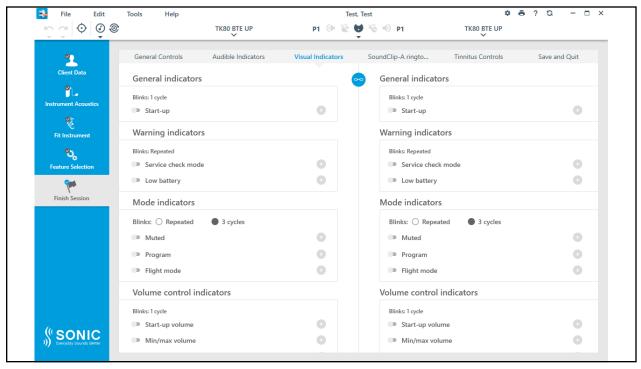


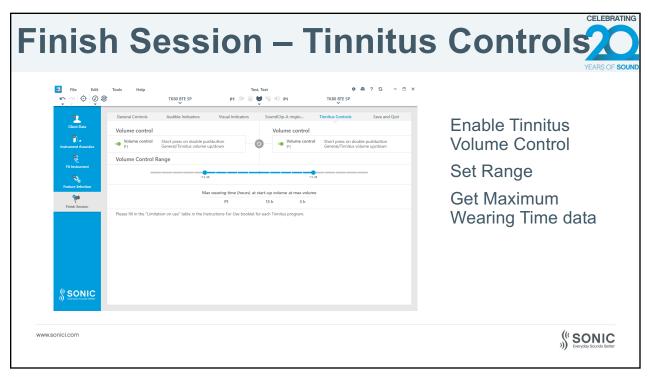


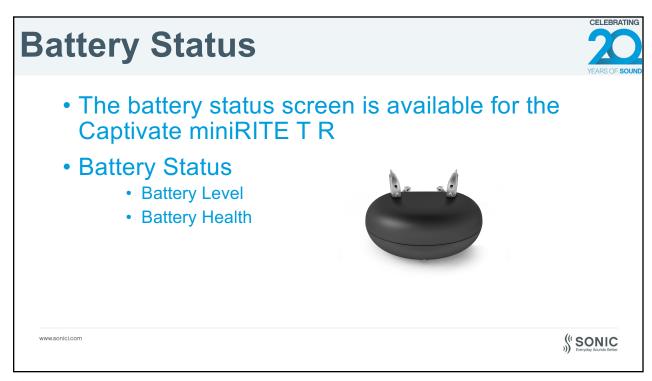

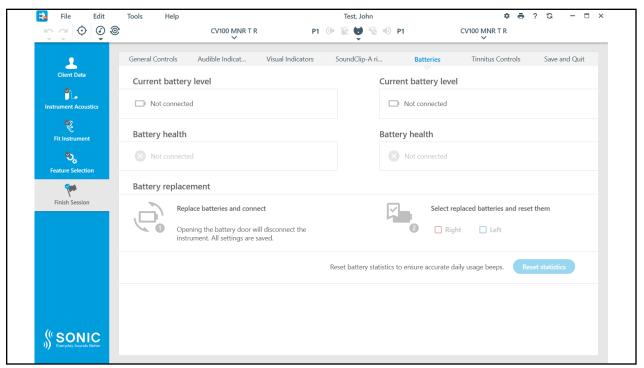

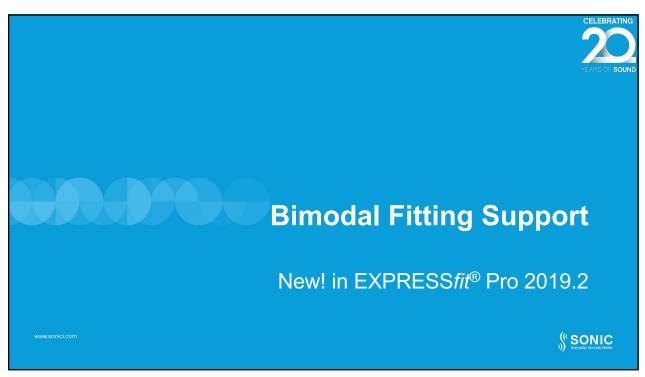

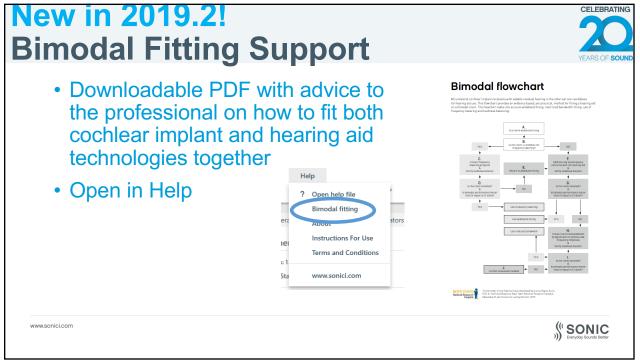

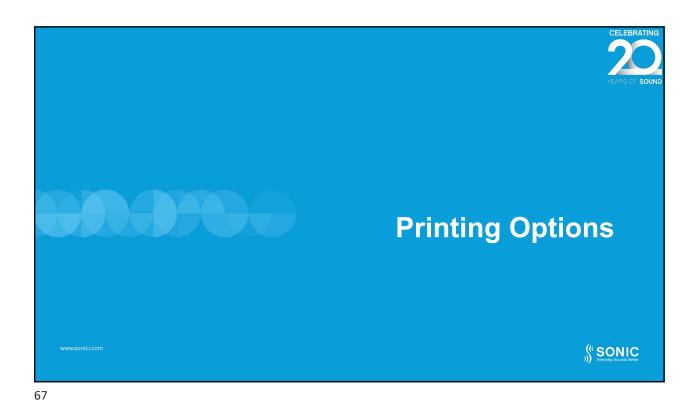

**Print Functions** 





- Client
  - Quick Guides
    - Hearing Instrument
    - SoundClip-A
    - Tinnitus settings
    - Customizable
    - Title Page option
    - Language selection

- Hearing Care Professional
  - Hearing Instrument settings
  - Customizable
    - HCP name
    - Company logo
  - Language Selection


www.sonici.com



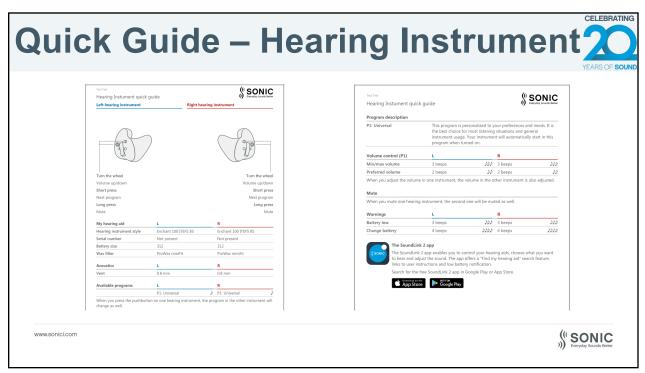


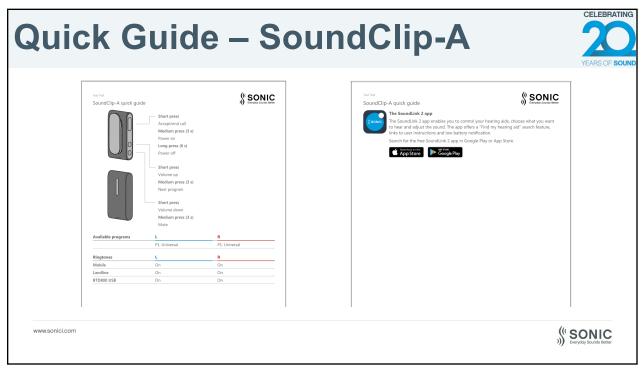



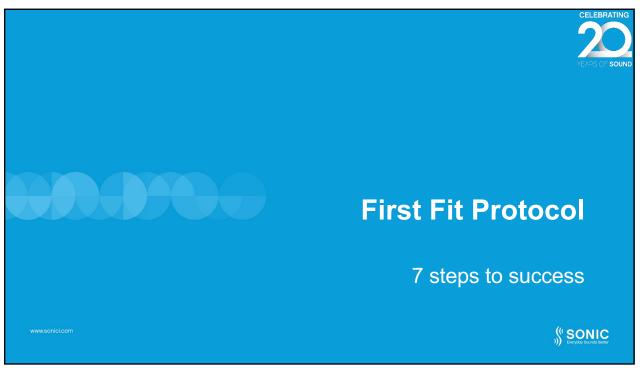

# First Fit Protocol 1. Edit Client Info • Verify demographics and fitting rationale 2. Adaptation Manager • Default is 80% 3. Program Manager 4. Run Feedback Manager

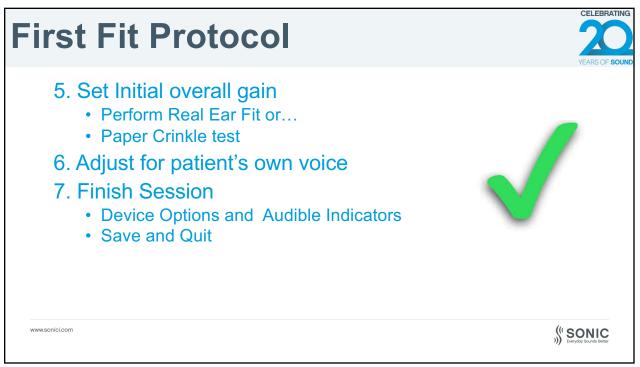

### **Final Comments**



- Thank you for joiningAny Questions? us today for our course
  - EXPRESSfit® Pro 2019.2: Not Your Mama's Fitting Software
- - 888.423.7834
  - www.sonici.com
  - www.mysonici.com
  - Email: support@sonici.com

www.sonici.com



